

Order details

UNYQ Client ID

Prosthetist

Patient/User ref.

Previous cover (s/n)

Notes

Common details

Design

Material

Firm

Prosthesis

AK/ TF

Coating

Glossy

Matte

Attachment

Magnets & Fast-clamp

Screws & C-Clamp

Colors

Global

Front

Back

Base

Detail

Extras

Engrave

Vinyl

Size
reduction

0 %

5 %


10 %

Measuring

Follow the instructions in the next page and fill in the requested measurements.


OneFit - Scanning Ordering

2 photos sound leg

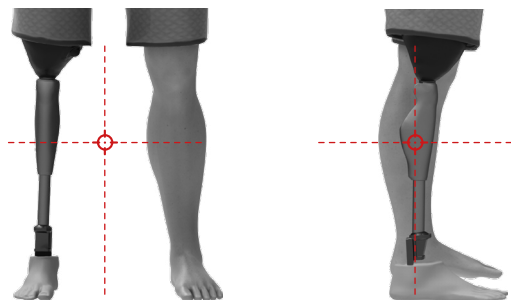


Take 2 photos of the user wearing the prosthesis, as shown in the images above. The camera must be placed perpendicular to the legs, in a low position, and both legs must be centered on the photo. Please remember that all prosthetic components must be completely visible, including the socket. Please remove shoes, socks and any object that covers the prosthesis.

2 measurements

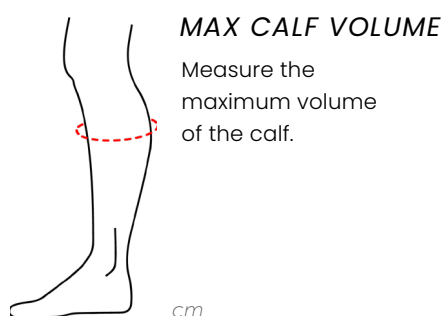

MAX CALF VOLUME

Measure the maximum volume of the calf.

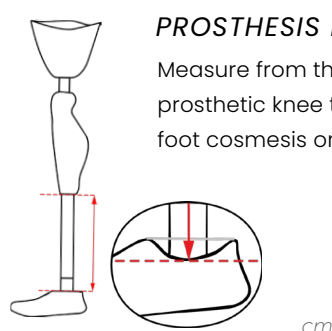

PROSTHESIS LENGTH

Measure from the bottom edge of the prosthetic knee to the top edge of the foot cosmesis on its lowest part.

Scanning



NO SHOES



NO SOCKS


.stl
.obj
FORMATS




STRUCTURED
LIGHT SCANNERS



COMPLETE
PROSTHESIS

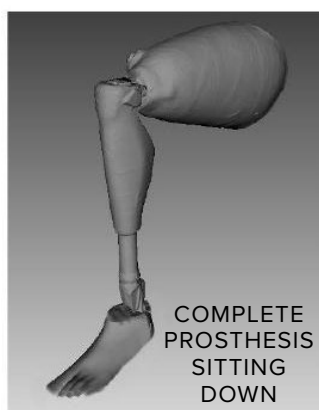

COMPLETE
PROSTHESIS
SITTING
DOWN

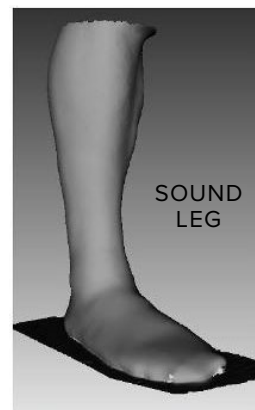

SOUND
LEG

- All prosthetic components should be clearly visible on the scan, including the lower part of the socket. Please remove any item that covers the prosthesis (sock, foam, other coverings ...)
- No reflecting ground: Avoid problems with reflective material or dark areas. If your scanner does not receive information from these areas, cover the reflective parts with matt tape, tightly taped to the surface so that it does not create extra bulk.
- We recommend that the environment contrasts in color with the prosthesis.
- Set the scanner to the highest resolution possible.
- Scan the complete prosthesis and the sound leg, with the patient standing up. You can scan both legs in the same file or do it separately.

Recommended scanner: Einstar Scanner; Shining 3D Einscan Pro Series Hand Scanners; Artec Structured Light Hand Scanners; Creaform Hand Scanners; Peel3d 3D Scanner.

Not recommended scanners: 3D Systems / Cubify Sense; Structure Sensor / Core; Microsoft Kinect 3D Scanner; Intel Infrared Sensor Scanners

SEND US THE FILES AND FORM

Send us this guide with the order details, measurements and photos to orders@unyq.com. If you need further assistance please contact us at orders@unyq.com or +34 854 85 60 92